

PPA3500 Series 1~6 Phase Power Analyzer



The Complete Solution for Variable Speed Drive Motor Development DUAL CORE

Product Overview				
1 to 6 Phase Configuration	Up to 6 Phase Analysis within 1 chassis			
Dual Core Power Processing	Enable dual analysis modes with maximum performance			
PWM Motor Drive Measurements	High Performance PWM Motor Drive Analysis			
Leading Wideband Accuracy in 2U form factor	0.04% Accuracy with class leading high frequency performance			
Wide Screen Display for 6 Phase Analysis	Unique wide aspect ratio for 6 Phase Analysis			
Market Leading Phase Accuracy	0.005 Degrees Phase Accuracy			
Built in High Precision Shunt	30Arms or 20Arms (LC) Internal Current Shunt			
Versatile interfaces	RS232, USB, LAN, GPIB, Torque, Speed and Extension for ADI40 Option			
Compact Size	Unique 6 Phase Power Analysis in 2U form factor			
Fast Sample Rate and No-Gap	1M sample/s			
Wide Frequency Range	DC & 10mHz to 1MHz			

PPA3500 Precision Power Analyzer

FRONT VIEW



1 POWER BUTTON

② FRONT USB PORT

USB memory port allows data or screendumps to be saved directly to a USB pen drive

③ WIDE ANGLE VIEW DISPLAY SCREEN

Double white LED backlit colour TFT display with high contrast and wide viewing angle

4 SCREEN DISPLAY OPTIONS

Zoom, Real time, Table and Graph options

5 MEASUREMENT FUNCTION SELECTION BUTTONS

- POWER ANALYZER
- HARMONIC ANALYZER
- TRUE RMS VOLTMETER and AMMETER
- OSCILLOSCOPE



Measurement Mode Control

6 MEASUREMENT SETTINGS BUTTONS

Acquisition settings - Sets wiring configuration,

Smoothing and data logging

Coupling - Set coupling to AC, DC or AC+DC, also set bandwidth

Range - Internal or external attenuator, autoranging settings, scale factors

Application mode - PWM, ballast, inrush current, power transformer, standby power,

Plus direct configuration of - Alarm, Auxiliary, Remote, System and Program functions

7 MENU SELECTION AND CURSOR CONTROL

8 START, STOP, ZERO AND TRIGGER

Trigger button refreshes measurement, Zero resets datalog or allows an offset trim Start and Stop buttons provide manual control of a measurement period



REAR VIEW



PPA3560 - 6 Phase

9 PHASE INPUTS

Direct voltage Input: 2.5kVpk (1kVrms) in 10 ranges

Direct current Input: 1000Apk (30Arms) Standard Model, 300Apk (20Arms) Low

Current Model in 10 ranges

External voltage and current sensor inputs to 3Vpk in 8 ranges - BNC Connector

10 SYNC CONNECTOR

Can be utilised for external triggering

11 EXTERNAL SENSOR INPUTS

+/-10V or pulsed input from torque and speed sensors provides direct measurement of mechanical power + analogue output

Extension Port: Connection of auxiliary devices such as the ADI40 40 Channel Analogue Input/Output Interface for Multi-Channel Sensor and Direct Thermocouple Measurement

12 PC INTERFACE CONNECTIONS

Standard interfaces: RS232 + USB + LAN

Optional Interfaces: GPIB


(13) Safety Earth Connection

Screw type safety earth connection




■ High Speed Power Measurement - 5ms Datalog Interval PPA3500

Measurements include all frequency components in power waveforms for example, fundamental, harmonics of the fundamental and the carrier of a PWM inverter output by maintaining 1Ms/s sampling at any drive frequency

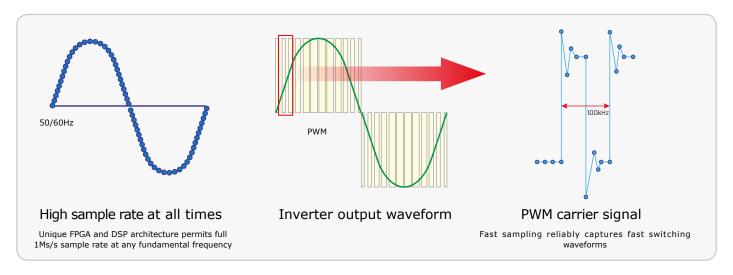


■ 1MHz Wideband Frequency Response PPA3500

With 1MHz bandwidth and exceptionally flat response, the PPA3500 provides precision analysis of total power in applications such as lighting ballasts or PWM drives that involve a wide range of frequency components. Proprietary to N4L, a digital process called Expanded Nyquist Sampling ensures no alias components.

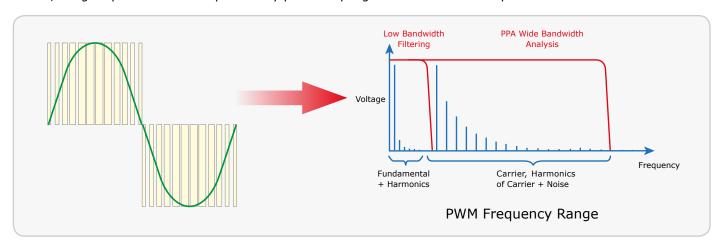


■ High Accuracy PPA3500

Unique voltage and current analogue card design ensures high accuracy for both power and harmonic analysis

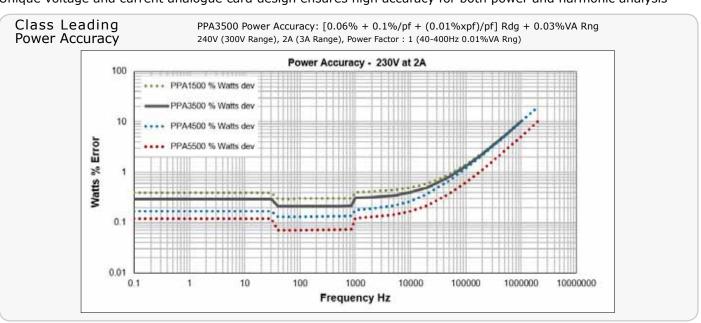

■ DFT Real Time No Gap Analysis PPA3500


Many power applications have fast changing asynchronous current pulses which are not suited to fixed data length FFT analysis. The PPA series combine a real time DFT (Discrete Fourier Transform) technique with variable window no gap analysis to ensure the optimum speed and accuracy at all times

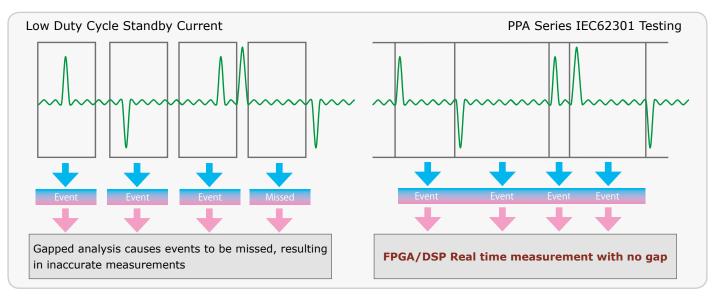

- Missing data compromises power accuracy
- Long term measurement integration achieves approximately correct average power
- Real Time No Gap analysis ensures correct power measurement
- Simultaneous fundamental and pulse frequency synchronization quickly obtains the correct power

■ Up to 6 Phase (8 Wire) Analysis PPA3500

The PPA3560 offers 12 channel, 6 Wattmeter measurements from a single chassis. All measurements are time synchronised utilising a central FPGA core which acquires the sample points from all 12 channels simultaneously, avoiding serialised data acquisition. This enables the PPA3560 to achieve unrivalled channel to channel phase angle accuracy and is one of the key contributors to the market leading 0.005deg phase accuracy.

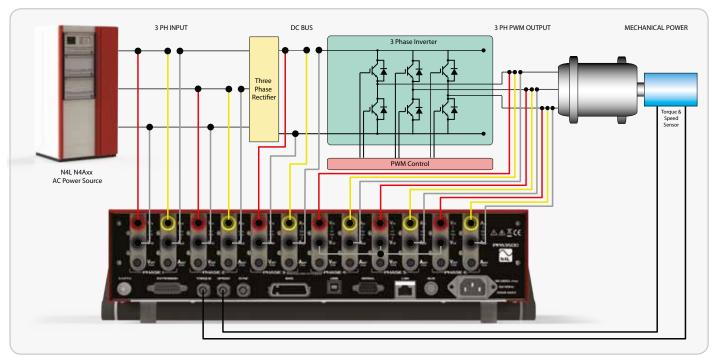

FPGA Core

- Simultaneous data acquisition, time synchronising phases
- High speed harmonic analysis
- True "Real Time" power computation with no gap

Measurement parameter examples

- Input/Output power measurement
- Efficiency of the inverter
- Inverter output voltage harmonics
- Motor drive characteristics

■ Input Torque and Speed Sensor PPA3500

Direct measurement of torque and speed from dedicated inputs that are fully synchronized with the voltage and current channels permits true real time power conversion efficiency to be evaluated



①TORQUE Isolated Bipolar±10V / pulsed
 ②SPEED Isolated Bipolar±10V / pulsed
 ③SYNC Isolated Bipolar±10V / pulsed

■ Built in Amplifier and Unique Shunt Resistor PPA3500



The PPA series use a single shunt resistor unique to N4L that combines exceptional linearity and no need for relay switching which can cause measurement errors

Model	Low Current Model	Standard Model
PPA3500	10 ranges: 10mApk - 30Apk (20Arms)	10 ranges: 30mApk - 1000Apk (30Arms)
PPA3300	10mΩ Shunt	3mΩ Shunt


External shunt options

(DC ~ 1MHz, 0.1% Accuracy, Inductance<1nH)

Model	Maximun	Maximum Current	
Model	Rated A	Peak	Bandwidth
HF500	500Arms	5000Apk	
HF200	200Arms	2000Apk	
HF100	100Arms	1000Apk	DC - 1MU-
HF020	20Arms	200Apk	DC \sim 1MHz
HF006	6Arms	60Apk	
HF003	3Arms	30Apk	






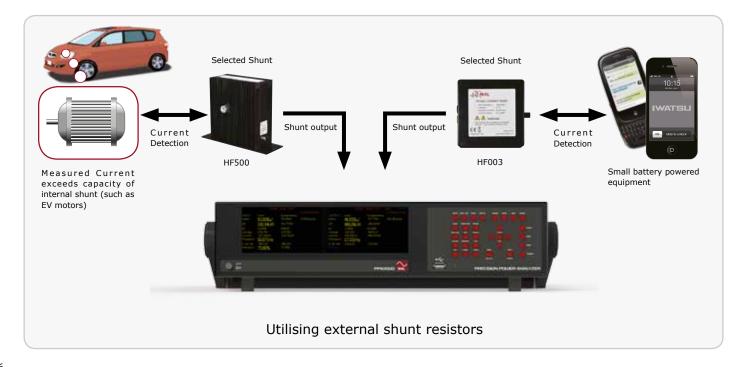

■ Power Analysis PPA3500

Wide Angle display for convenient viewing of 6 Phase Power Analysis

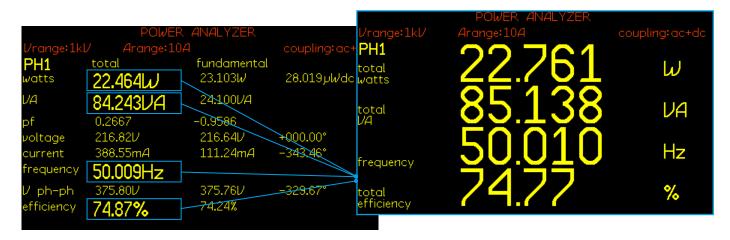

Zoom function enabled on total watts, total VA, frequency and total efficiency

	POWER ANALYZER				
watts	phase 1 23.142	phase 2 11.967	coupling: c phase 3 27,226	ic+dc W	
VΑ	85.827	56.944	94.807	VΑ	
pf	0.2696	0.2102	0.2872		
Urms	217.62	219.16	219.91	ν	
Arms	394.39m	259.83m	431.11m	А	
frequency	50.013			Hz	
V ph−ph	377.13	380.26	379.21	ν	
efficiency	74.80%				

3 Phase analysis display

All power measurement and RMS values are computed simultaneously across 6 phases, allowing measured values to be selected and viewed during analysis.

Here, three phase input and 3 phase output power can be selected with all primary power functions in each phase plus frequency, a selected harmonic, dc watts and phase to phase voltage

Mechanical power, Maths and Efficiency functions can also be added to this screen giving real time analysis of electrical or electrical to mechanical systems


MEMORY

Large 500MB internal memory, data logging from 5ms intervals with synchronization to the fundamental frequency and no gap between measurements

Datapoint storage up to 5M

Alternatively the data can be stored in an external USB pen drive or directly to PPALoG PC software

Voltage, Current, Frequency and Power - Examples of graph mode

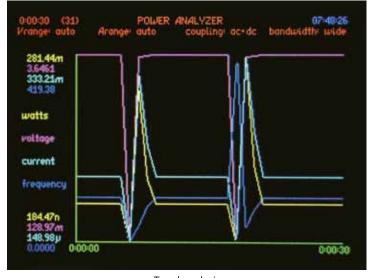

■ Power Integrator (power consumption) Mode, RMS Meter Mode and Impedance Meter Mode PPA3500







Power Integrator mode

RMS Voltmeter mode


Impedance meter mode

Note

In addition to detailed measurements of the phase power parameters, you can check the balance of power between the phases and observe computed neutral current when 3 phase 4 wire connection is selected, this can be performed over 6 phases with 3 Phase 3 Wattmeter + 3 Phase 3 Wattmeter wiring configuration.

■ Harmonic Analyzer and Oscilloscope PPA3500

In Harmonic Analyzer Mode, the PPA3500 provides up to 100 Harmonics with real time, table or bar graph presentation. Measurements are in absolute magnitude and percentage of fundamental with harmonic phase also available. The Discrete Fourier Transform (DFT) is utilised, resulting in highly accurate harmonic analysis. With accuracy figures matching the headline Voltage and Current specification the PPA3500 is a highly capable harmonic analyzer. The use of the DFT is made possible via high speed parallel FPGA signal processing as well as proporietary low level DSP algorithms. The DFT was selected for signal decomposition due to the fact that sample by sample window resolution is possible, instead of the restrictive 2ⁿ sample window size of the FFT, the DFT is capable of minimal leakeage without the need of error prone window filtering functions.



Harmonic analyzer (Bar graph)



Harmonic analyzer summary page



Harmonic analyzer table


Vrange:1kV	OSCILLOSCOPE Arange:3A	coupling:ac+dc
PH2 voltage	\sim	
current	Anatanaliaspina	لتجينا
5.000ms/div		

Oscillosope - Voltage and Current display



Three phase display of voltage

Harmonic Accuracy		
Voltage	0.04% Rdg+0.1% Rng+(0.005%×kHz)+5mV	
Current	PPA3500-LC 0.04% Rdg+0.1% Rng+(0.005%×kHz Rdg)+300uA PPA3500 0.04% Rdg+0.1% Rng+(0.005%×kHz Rdg)+900uA	

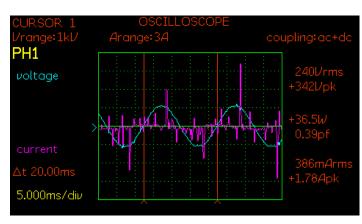

Oscillosope Cursors - Enable cursors and display Vrms, Vpk, Watts, Power Factor, Arms and Apk

ACQUISITION SETTINGS

■ Auto-Ranging, Range Up Only or Manual PPA3500

Range modes are selectable

①Auto-Ranging Performs automatic switching of voltage and current ranges up and down depending on the level of

the measured value with all inputs linked or ranged independently to ensure optimum accuracy

②Range up only Performs automatic ranging when the input is 120% of range, ranging up only


③Manual No automatic ranging, user specifies the range in which to operate


(used when input voltages and currents are known) or during inrush current testing

■ Independently Set Input Coupling PPA3500

Independently set input coupling so different methods of sensing can be implemented. Such as CT's on phase 1+2, resistive shunt sensing on phase 3 and Rogowski coils on phase 4~6.


> **AC Waveforms** DC Waveforms



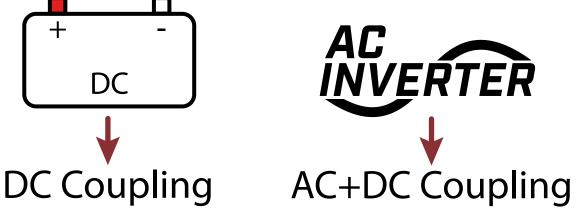


AC+DC and DC coupling both provide 1MHz bandwidth measurements, the coupling setting ensures the instrument is synchronised to the largest power component of the measured waveform. DC coupling should be used for DC bus measurements and AC+DC coupling used for Inverter Output and AC input power measurements.

■ Wiring Settings PPA3500

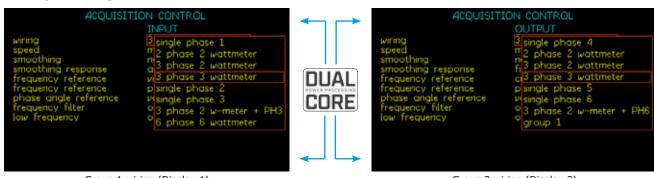

Group 1 wiring (Display 1) Group 2 wiring (Display 2)

The PPA3500 utilises a dual control menu system, the instrument is divided into 2 distinct groups. Group 1 is controlled via display 1(left hand) and group 2 is controlled via display 2(right hand).

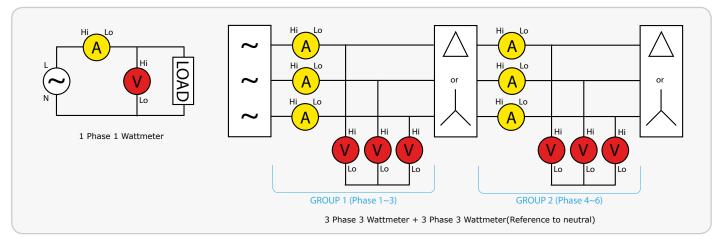

ACQUISITION SETTINGS

■ Bandwidth Settings PPA3500

Low(DC-200kHz) Basic power (50/60Hz) including

harmonics of the fundamental while

rejecting high frequency noise

Wide(DC-1MHz) Wideband applications such as PWM

> inverter drives including all power components for true total power



Example of wiring configuration showing 1 phase, individual coupling settings also available.

The PPA3500 series includes a programmable digital filter that allows users to set a preferred bandwidth

■ Display Settings, Smoothing Response and Frequency Reference PPA3500

1) Display update rate

Various settings for the display update rate (5ms \sim 100s) which also increases the smoothing when used together with the smoothing option. A 'window' option permits direct control of the measurement window size





Example of setting the window, eg (100Hz set to 10ms)

2Smoothing settings

Working in conjunction with the speed setting, a smoothing filter can then be applied to the measurements. Normal and slow options are available which apply an increasing time constant to the output of the measurement window




speed	update rate	normal time constant	slow time constant
Very Fast	1/80s	0.05s	0.2s
fast	1/20s	0.2s	0.8s
medium	1/3s	1.5s	6s
slow	2.5s	12s	48s
very slow	10s	48s	192s

- Display update speed settings
- Setting the filter (normal/slow)

Frequency Reference PPA3500

When making a precision measurement of ac power, correct synchronization with the fundamental frequency is essential. The PPA series provides a solution to frequency synchronization in a wide range of applications including Standby Power, Variable Speed Drives, Electronic Ballasts and DC to AC Inverters with the option to select voltage, current, speed or ac line input as the frequency reference.



Frequency Reference

■ Simultaneous Dual Mode Capability



The PPA3500 has the capability to output two modes simultaneously utilising N4L's proprietary "Dual Core Power Processing" Architecture, providing great flexibility to the user. Of particular interest is the ability to display both Power Analysis and Oscilloscope data at the same time, while maintaining full sample rate. Traditionally, it is common for instruments to decrease raw sample rate within the power analyzer function when another mode is enabled. The PPA3500's "Dual Core" architecture allows for maximum performance of both modes.


Example Dual Core Operation



APPLICATIONS


■ PWM Motor Drive Evaluation PPA3500

The PPA3500 is the ideal solution for 6 Phase Analysis within a single instrument, a typical application is Variable Speed Inverter Drive analysis. Utilising proprietary digital filtering algorithms, the N4L power analyzer range offers unrivalled performance. The PPA3500 can be used in conjunction with external current sensors such as the WR5000 - a 1MHz 5000A Rogowski Coil in high current applications as well as the LEM range of Zero Flux Current Transducers. Inverter efficiency is available via 3 Phase 2 Wattmeter method + CH3 + 3 Phase 3 Wattmeter, whereby PH1+PH2 are utilised to measure the input power to the three phase rectifier, PH3 is used to monitor DC bus power and PH4~PH6 are used to monitor the output power of the variable speed inverter drive.

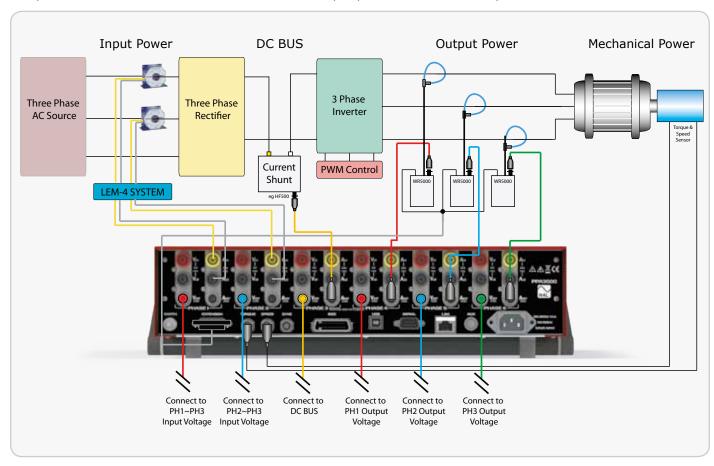


■ High Speed Analysis PPA3500

The PPA3500 features high speed parallel digital signal processing, this enables high speed tracking of changing inverter drive frequencies and power parameters during ramp up and ramp down conditions, for example in electric vehicle applications. N4L's free to download software package (PPALoG) offers datalog intervals down to 5ms, providing fast, no-gap real-time data direct to software.

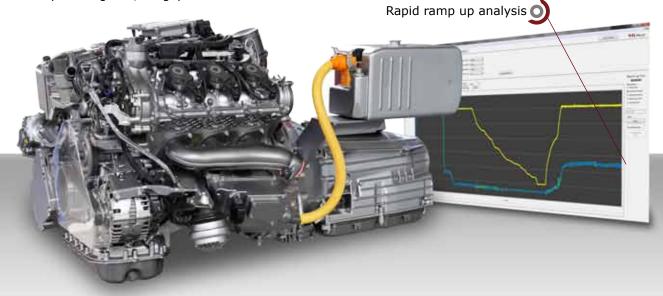

■ 4 Phase Solar Inverter Performance Analysis PPA3500

The PPA3500 provides a highly accurate solar inverter analysis and evaluation solution from one measurement chassis, featuring independent frequency detection N4L Power Analyzers exhibit the ability to synchronise to the 50/60Hz output signal simultaneously with the DC input signal from the solar array. Both efficiency of the inverter, quality of the AC output and many other performance parameters can be recorded. In the application below, the PPA3500 is configured as a 4-Channel solution which allows the user to display DC Input to 3 Phase output efficiency data along with THD power quality measurements from one measurement chassis.

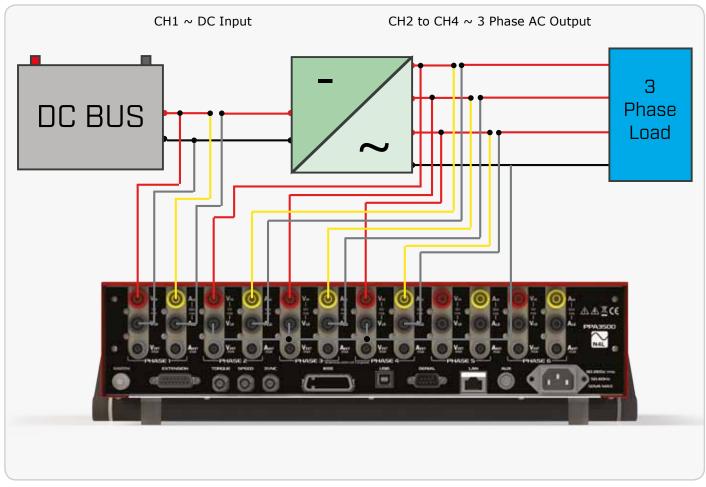


■ Inrush Current PPA3500

Accurate inrush current measurements rely upon two factors aside from fundamental measurement accuracy, these are gapless measurement and a high sampling rate;

- 1. Gapless Measurement Inrush waveforms by their nature are transient; gapless measurement is vitally important in order to ensure that inrush waveform data is not missed.
- 2. High Sampling Rate When working with mains frequencies, many power analyzers have low sample rates due to the computation of measured values from a data block of finite size. The PPA3500 utilises a proprietary real time signal processing technique that maintains full 1Ms/s sample rate irrespective of the measured load frequency, ensuring that high frequency events are captured without aliasing.

Example Inrush current data, datalogging at nominally 20ms intervals directly to PPALoG



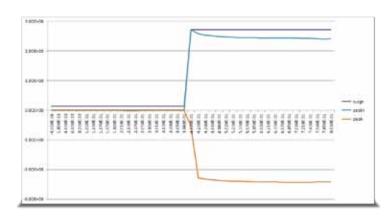

Calibration and ISO17025 Certification

UKAS PPA3500



Newtons4th are an accredited UKAS Calibration laboratory, all PPA3500 Power Analyzers are supplied with an ISO17025 UKAS Calibration Certificate as standard. Calibration of N4L Power Analyzers is an integral and important part of our service to our clients, we offer quick turnaround times at a competitive price. Re-Calibration is also available at our international offices and various distributors throughout the world*.



■ Schedule of Accreditation PPA3500

N4L's schedule of accreditation to ISO17025 is wide ranging and an overview of the schedule is detailed below, for more specific information please see the UKAS website to view the full accreditation schedule.

	ISO17025 UKAS Accreditation Schedule				
	Signal Amplitude	Frequency Range			
Voltage Sine Amplitude	1V to 1008V	16Hz to 850Hz			
Voltage Harmonic Amplitude	0V to 302V	16Hz to 6kHz			
Current Sinewave Amplitude	t Sinewave Amplitude 100mA to 48A 16Hz to 850Hz				
Current Harmonic Amplitude	0A to 15A	16Hz to 6kHz			
Current to Voltage Phase Angle	-180° to +180°	16Hz to 850Hz			
Apparent Power (VA Product)	100mVa to 48.4kVA	16Hz to 850Hz			
AC Power	0W to 48.4kW	16Hz to 850Hz			
AC Power (Calorimetry) 1W to 5W 45Hz to 2MHz		45Hz to 2MHz			
Current Harmonic Amplitude to IEC61000-4-7	0A to 6A	16Hz to 6kHz			
	Pinst(Sinusoidal Modulation)				
	Pinst(Rectangular Modulation)				
	Pst				
Filebrane IFCC1000 4 1F	Frequency Changes	Ac now IEC61000			
Flicker to IEC61000-4-15	Distorted Voltage with Multiple Zero Crossings	As per IEC61000			
	Harmonics with Sidebands				
	Phase Jumps				
	Rectangular Changes with Duty Cycle				





■ Guaranteed Accuracy up to Crest Factor 20

The Newtons4th Power Analyzers feature a guaranteed accuracy up to a crest factor of 20, meaning the autoranging system of the PPA3500 is able to peak detect automatically upon waveforms with a crest factor (peak/rms) of up to 20.



Newtons4th are the only Power Analyzer Manufacturer in the world** to provide ISO17025 calibration certficates on all new Power Anlayzers as standard. Our ISO17025 Schedule of Accredition includes Voltage, Current, Phase, Power, Harmonics and Flicker. With traceable certification of power accuracy down to 0.5W, N4L offer the ideal measurement solution for certified standby power measurement.

Due to the specialist nature of Power Measurement Instrumentation Calibration, N4L utilise both commercially available calibration equipment (such as the Fluke 6105A for UKAS Certification) along with N4L bespoke designed signal generation equipment in order to calibrate our instruments over the full frequency range (up to 2MHz). Calibration over the full frequency range is uncommon given that such signal generation equipment is not commercially available. When supplied with an N4L analyzer, all customers will receive a calibration certificate covering the complete frequency range.




^{*}N4L's UKAS ISO17025 Laboratory is based in the UK, international accreditation is dependent upon local distributor calibration capabilities

**According to N4L research, 2015

Ranging Principles

■ 10 Stage Solid State Ranging System - PPA3500

Combining highly linear voltage attenuator and current shunt designs with a proprietary 10 stage solid state ranging system on every phase input, the PPA series achieve a uniquely wide dynamic range, with no need to switch between voltage attenuators or current shunts when ranging up or down.

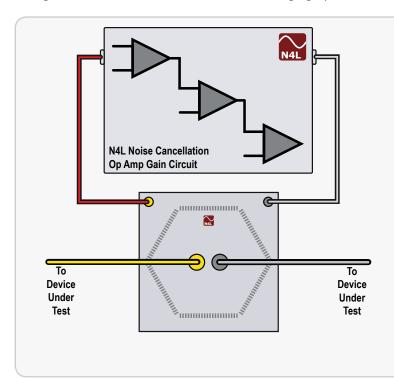

Design features:

Auto DC offset trimming

Single attenuator on each voltage input
High impedance low capacitance
Single shunt on each current input
Low impedance low inductance
Auto peak detect
High speed solid state ranging
High Noise rejection


Benefits:

Overload protected on any range
Low shunt affect on voltage connections
Low voltage burden on current connections
Market leading phase accuracy
Peak detect ranging ensures no signal clipping
Low attenuator/shunt operating temperature
Fast range switching
Constant frequency response on all ranges
Signal can be applied with instrument powered off

■ Auto Peak Ranging Ensures Complete Waveform Analysis PPA3500


It is often overlooked that for an instrument to correctly calculate power parameters, the entire waveform must be digitised for analysis. The Peak Ranging system employed by all N4L Power Analyzers ensures that the entire waveform is digitised and the correct power parameters are calculated.

Example RMS Ranging system, commonly used in older instrument designs

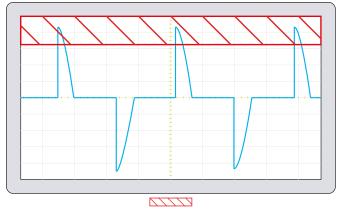

Waveform within red hashed area is clipped by an RMS ranging system and fixed crest factor setting

Modern Peak Ranging System, implemented on all N4L Power Analyzers

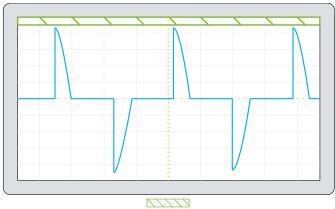

Peak Ranging system auto-detects the peak of the input signal and selects the ideal range

Note


An RMS Ranging system requires the user to have prior knowledge of the crest factor which in many applications is not practical, either because the user cannot reasonably be expected to know this value before a measurement, or because the crest factor is changing during a measurement period. The ideal ranging system is therefore based upon peak detection which does not require the user to be concerned with a crest factor setting. While many RMS ranging systems are only guaranteed to support a Crest Factor of 6, all N4L Power Analyzers guarantee to auto-range with any crest factor and maintain full accuracy with a CF of at least 20. While waveforms with a true CF above 20 are very unusual, 'auto range up' or 'manual' ranging combined with a market leading range sensitivity enables the PPA to achieve a dynamic range equal to a CF >300.

PC CONTROL AND DATA ACQUISITION


■ PC Software PPA3500

Analysis carried out by the instrument can easily be transferred to a PC via USB, RS232 or LAN

① **PPALoG** Exceptional flexibility and ease of use with all the functions included in the original PPAcomm program plus multiple instrument control for 7-24 phase applications and data export to Text file, Excel, Bitmap or Clipboard

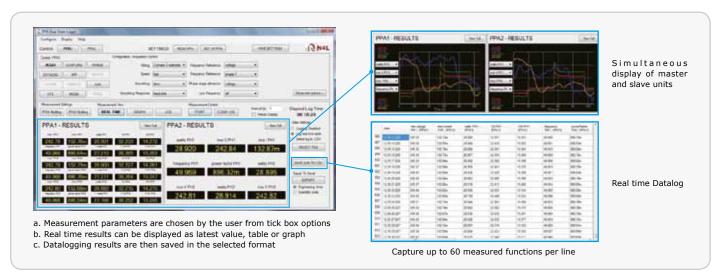

Data Export options

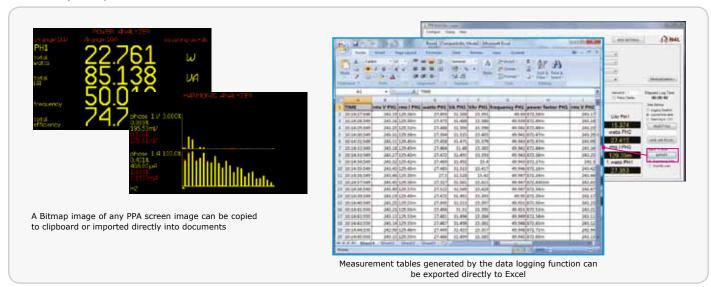

② **PPA Standby Power** Full compliance testing to EN50564 (IEC62301). Meets or exceeds the requirements and methodology of U.S. EPA (Energy Star), U.S.DOE, California Energy Commission (CEC), among others.





Standby power test screen with real time update of EN50564 (IEC62301) criteria

		Ped Greatly		
Division Leader Teach				
in trad	Conference ABC			
Victel	125.450			
tend 70.	1380			
bread Nobige Arrang	2006			
Sales County (Security)	230m N			
Sal Hills Square Us. (3-5)	CHERN			
appd (cyst (o))	440			
). (I mean	Court on OUT year	na no haban man		
Final Review of Prof.				
All Marris	26.46			
antico.	Mount sorrel, Long	houseach, 1727	ST. U.C.	
11 e	1 9/36 /889			
las	WAR.			
CONTRACTOR OF	12.0			
4 mile y	102			
THE PIC	L			
(series)	Dependency w	M. 859		
Marana meni kemanan di		nen		
Versillarium.	95000 90004			
Works	9942360 Applica			
Secol Sc.	176			
thi carbins	1.75			
- III CARRESTE		el como medidade		
or tages of	50002	1111011001001000		
Face array (Md)	15,803			
- Bro Brown and	Michigana Adai	Lame Local	Operation's	"13 Res.4.
Andrew Comments	0.0872016	2	2	P4/5
Services	14003	·.M.	145	PAGE
ar-rate		mi Keralia	145	F-900
		alkasu.		
Yorker	233628			
Arms Mari	2530645 273040			
ing hour larger	03005			
ky marchi franc (NA)	1.79315			
	15/805			
Supply Free comp (44)				
coed Darry Lytin (18)	40.2515			
Joed Dany Lyttle (18) Dagmer Time (1997-19)	40,2275			
coed Darry Lytin (18)	00400			
Joed Dany Lycis () is: (higher Time (nor in) (to all,) Pares	State and white		Openiore	Ten (teach
oad Dery Lyce (ries (laguer line (merie) (la site, Pares Sener (A.)	Gent Manager value 1.03004	117009	3.15577	CTURK
oad buy (yes) is (lapser line (nor e) (to sto Pers (mar (A) (nor Park)	Manufact white 1 (2004) 1 (2004)			
oad Dery Lyce (ries (laguer line (merie) (la site, Pares Sener (A.)	Gent Manager value 1.03004	117009	3.15577	CTURK

On completion of the standby test, a full test report can be exported directly to a spreadsheet

SPECIFICATION

				PPA3500		
Frequenc	y Range					
1	Normal	PPA3500-LC(20Arms) DC,10mHz \sim 1MHz, PPA3500(30Arms) DC,10mHz \sim 1MHz				
		Range 1+2* ** : DC, 10mHz ~ 100kHz				
Np. of Ph	ases					
)				1~6		
Voltage I	nput Range		Normal :	100 mVpk \sim 2500Vpk(1000 Vrms) in 10 ranges (240 Vrms within	300Vpk range, using 20% overange)	
Internal	Accuracy			1V ~ 2500Vpk range : 0.04% Rdg+0.1% Rng+(0.005	%×kHz Rdg)+5mV	
				Range 1+2*: 0.04% Rdg+0.1% Rng+(0.01%×k	3,	
External ⊢	Range Accuracy			1mVpk ~ 3Vpk in 8 ranges [BNC connector 3Vp 0.04%Rdg+0.1%Rng+(0.005%×kHz Rdg		
Current I				0.0 . /	, , , , ,	
		20Arms Low Current	Ranges	10mApk ~ 300Apk(2	· · · · · ·	
		(PPA3500-LC) 4mm safety connectors	Accuracy	, 3	10mA** ~ 30mA** ranges: 0.04% Rdg+0.1% Rng+ (0.01%×kHz Rdg)+100μA	
			Ranges	30mApk ~ 1000Apk(
		30Arms (PPA3500)		300mA ~ 1000Apk ranges:	30mA** ~ 100mA** ranges:	
		4mm safety connectors	Accuracy	, ,	0.04% Rdg+0.1% Rng+(0.01%×kHz Rdg)+ 300μA	
External in	nnut		Ranges	1mVpk ∼ 3Vp	k in 8 ranges	
(External	•	BNC Connector (Max input 3Vpk)	903	1111 PK 34		
Current se	ensor)	рас этрку	Accuracy	0.04% Rdg+0.1% Rng+(0.005%×kHz Rdg)+ 3μV	
Phase Acc	curacy					
				Normal: 0.005deg+(0.01deg×kHz) Range 1+2* ** : 0.	005deg+(0.02deg×kHz)	
Power Ac	curacy					
				[0.1% + 0.1%/pf + (0.01%xkHz)/pf] Rdg + 0	-	
				Range 1+2* ** : [0.1% + 0.1%/pf + (0.02%xkHz)/pf]	Rdg + 0.05%VA Rng	
40-850Hz	!			[0.06% + 0.1%/pf + (0.01%xkHz)/pf] Rdg + 0.000	0.03%VA Rng	
General						
Crest Fact				20(Voltage and Current)		
Sample Ra				1Ms/s on all channels, No-Gap	ny Chau	
IEC Modes		IEC50564 (Replaced IEC62301) and Energy Star PWM Motor Drive, Ballast, Inrush, Power Transformer, Standby Power				
		Mode Rejection Ratio				
		250V @ 50Hz - ≥ 1mA (150dB)				
Maacuran	mont Dar	100V @ 100kHz - ≥ 3mA (130dB)				
Measuren	nent rais	meters W, VA, Var, pf, V & A - rms, rectified mean, AC, DC, Peak, Surge, Crest Factor, Form Factor, Star to Delta Voltage, +ve Pk, -ve Pk				
		, ,	, , ,	Frequency (Hz), Phase (deg), Fundamentals,		
				Harmonics, THD, TIF, THF, TRD, TD		
Datalog	Un to 4	usar salastable measur	amont fun	Integrated Values, Datalog, Sum and Neutr		
Datalog W		user selectable measure	user selectable measurement functions across 6 phases, 32 total (60 with optional PC software) No-Gap analysis, Minimum window 5ms			
Memory				500MB, 5M records		
Communi	ication Po	orts				
RS232 LAN				Baud rate up to 38.4kbps,RTS/CTS flow 10/100 Base-T Ethernet auto sensin		
GPIB				(Option G - External Adapter) IEEE488.2 Co		
USB				USB 2.0 and 1.1 Compatible		
Analogue				Bipolar ±10V(BNC)	0.010/ D.L.	
Speed Inp Torque	out			BNC Bipolar±10V or Pulse count 1Hz to 1MHz BNC Bipolar±10V or Pulse count 1Hz to 1MHz	•	
Standard	Accesso	BNC Bipolar±10V or Pulse count 1Hz to 1MHz 0.01% Rdg ries				
Leads				Power, RS232, USB		
Connectio	n Cables			36A 1.5m long 4mm stackable termin		
Connectio	n Clips		1x red, 1x yellow and 2x black per phase 4mm terminated aligator clips - 1x red, 1x yellow and 2x black per phase			
CD-ROM				CommView2 (RS232/USB/LAN), Command line, Script based		
Document				Communications manual, Calibration certificate, Q	uick start guide	
Mechanic Input Imp		onmental		Voltage Attenuator and External Inputs 3.3M	O II 25pF	
Display	reudiice			2 x 480x272 dot full colour TFT, White LED		
Dimension	ns			92H x 404W x 346D mm excluding fe		
Weight				5.9kg(3 Phase), 8.8kg(6 Phase)		
Safety Iso				1000Vrms or DC(CATII), 600Vrms or DC(·	
Power sup		2200	E°C 41	90 ~ 265Vrms, 50 ~ 60Hz, 50VAma		
Operating Conditions		23 C ±	5 CAMb	ient Temperature (or air intake temperature when rack mounted Temperature coefficient ±0.01% per °C of reading at 5		
				Note *: Voltage Range[x] 1 + 2 : [1]100mV + [2]300		

Note * : Voltage Range[x] 1 + 2 : [1]100mV + [2]300mV

Note ** : Current Range[x] 1 + 2 : PPA3500-LC 20Arms model: [1]10mA + [2]30mA , PPA3500 30Arms model: [1]30mA + [2]100mA

SPECIFICATION

	PPA3500
Harmonic Specific	ation
Bandwidth	DC,10mHz ~ 1MHz - PPA3500-LC(20Arms), PPA3500(30Arms)
No. of Harmonics	100
Sampling Frequency	1Ms/s
Signal Processing	DFT (Discreet Fourier Transform)
Crest Factor	20
Power Factor	0 to 1
Harmonic Accurac	у
Voltage	0.04% Rdg+0.1% Rng+(0.005%×kHz Rdg)+5mV
Current	PPA3500-LC 0.04% Rdg+0.1% Rng+(0.005%×kHz Rdg)+300uA PPA3500 0.04% Rdg+0.1% Rng+(0.005%×kHz Rdg)+900uA
	Harmonic Accuracy (above) still applies with Frequency Filter set
Cycle by Cycle Ana	lysis direct to PC - 2Ms/s sample rate (Window setting)
Data Rate	10ms (all channels active)
	lysis direct to Internal RAM - 2Ms/s sample rate
Data Rate	5ms (all channels active)
20ms	Overload Capability 4.2kVpk (3kVrms)
5s	3.1kVpk (2.2kVrms)
Continuous	3kVpk (1kVrms)
Voltage Attenuator	
Current Shunt Imp	edance
20Arms	10mΩ
30Arms	3mΩ
Selectable Analgou	
	250kHz
	leasurement at Full Accuracy
PPA3500-LC	220uArms
PPA3500	700uArms

ACCESSORIES SUPPLIED AS STANDARD

Leads and Interfacing				
Туре	Specification			
36A Connection lead set	1.5 Metre - 36A lead set with 4mm stackable safety terminals $1x$ Red, $1x$ Yellow and $2x$ Black per phase plus alligator clips			
RS232 cable	RS232 9pin serial Cable			
USB cable	USB 2 Metre A male to B male			
LAN Interface	LAN fitted as standard			
USB to 9-pin RS232 (Option)	USB ~ 9-pin RS232 Serial Converter			
GPIB Option	GPIB Interface Option			

OPTIONAL ACCESSORIES

PC Software (Optional CD, Free to Download)					
Туре	Specification				
PPALoG	PC control and data acquisition of 1 \sim 24 phases with selectable Real Time data, Graphing, Datalog and versatile export options User Manual for PPALog available as a free download from our website				
PPA Standby Power	Standby power measurements and reporting to IEC62301				

Carry cases (Optional)					
Туре	Specification				
Soft carrying case	Black nylon with shoulder strap				

Documents (Standard)						
Type Specification						
Calibration/Test & Inspection Certificate	PPA Certificate of Calibration					
UKAS ISO17025 Certificate	UKAS ISO17025 Certificate of Calibration					
	Quick Start Guide					
Spare set of manuals	Comms manual					
	PPALoG user guide available as website download					

Connection and extension port accessories (Optional)				
Type Specification				
Breakout box	Simple analyzer connection between source and DUT			
PCIS	10Arms 300Apk rated Phase Controlled Inrush Switch			
ADI40	40 Channel Analogue Input/Ouput Interface			
GPIB Communication GPIB Communication Gettle Option				
Cable	GPIB Communication Cable Option			

Breakout Box



Rack Mount Kit (Optional)					
Туре	Specification				
Rack Mount brackets	PPA3500 19in rack mount brackets				

Interface (Optional)	
Type	Specification
PPA-GPIB interface	Option G - GPIB(IEEE488)Interface

ACCESSORIES

High Performance Voltage Attenuating Probes						
Model	Voltage Range	Frequency Range	Details			
TT-HV250	2500Vpk	300MHz	High Voltage Probe (Passive) 2.5kVpk 100:1			
TTV-HVP	1500Vpk	50MHz	High Voltage Probe (Passive) 15kVpk 1000:1			
ATT10 30Vpk 30		30MHz	10:1 Voltage Attenuator Box (For use in conjunction with HV Probes when output voltage of probe is >3Vpk, BNC			
		3011112	Input/BNC Output)			
ATT20	60Vpk	30MHz	20:1 Voltage Attenuator Box (For use in conjunction with HV Probes when output voltage of probe is >3Vpk, BNC			
ATTZU	συνρκ	3UMUZ	Input/BNC Output)			
ULCP	3000Vpk	2MHz	1000:1 Ultra Low Capacitance Probe (Active), For use in applications such as Ballast Testing (<1pF Capacitance)			





TT-HVP 15kVpk Probes





High Performance External Current Measurment Options								
Model Number	Measuring Range	Frequency Range	Basic Accuracy	Phase Accuracy	Details			
HF003	3Arms - 30Apk	DC - 2MHz	470mΩ (±0.1%)	0.0001° / kHz	3Arms External Current Shunt, BNC Output (Use with PPA External Input)			
HF006	6Arms - 60Apk	DC - 2MHz	100mΩ (±0.1%)	0.001° / kHz	6Arms External Current Shunt, BNC Output (Use with PPA External Input)			
HF020	20Arms - 200Apk	DC - 2MHz	10mΩ (±0.1%)	0.01° / kHz	20Arms External Current Shunt, BNC Output (Use with PPA External Input)			
HF100	100Arms - 1000Apk	DC - 2MHz	1mΩ (±0.1%)	0.05° / kHz	100Arms External Current Shunt, BNC Output (Use with PPA External Input)			
HF200	200Arms - 2000Apk	DC - 2MHz	0.5mΩ (±0.1%)	0.1° / kHz	200Arms External Current Shunt, BNC Output (Use with PPA External Input)			
HF500	500Arms - 5000Apk	DC - 2MHz	0.2mΩ (±0.1%)	0.1° / kHz	500Arms External Current Shunt, BNC Output (Use with PPA External Input)			









ternal Shunt HF-003	External Shunt I

External Shunt HF-200

External Shunt HF-500

Probe/Current Clamp Transformer: AC								
Model Number	Measuring range	Frequency range	Accuracy	Details	Clamp diameter	Category		
M3 UB 50A-1V	100mA ∼ 50A	40Hz ∼ 5kHz	1%	100mA to 50A AC Current Clamp	15mm×17mm	600V CATIII		
M3 U 100A-1V	1A ~ 100A	40Hz ∼ 5kHz	1%	1A to 100A AC Current Clamp	15mm×17mm	600V CATIII		
S UE 200A-1V	1A ~ 200A	40Hz ∼ 5kHz	1%	1 A to 200A AC Current Clamp	50mm ø	600V CATIII		
S UE 250 500 1000-1V	1A ~ 250A/500A/1000A	40Hz ∼ 5kHz	1%(250A) 0.5%(500+1000A)	1 A to 250/500/1000A AC Current Clamp	50mm ø	600V CATIII		
US UE 1000A-1V	1A ~ 1000A	40Hz ∼ 5kHz	1%	1A to 1000A AC Current Clamp	43mm ø	600V CATIII		
SM UE 1000A-1V	0.5A ~ 1000A(1%>100A)	15Hz ∼ 15kHz	1%	0.5A to 1000A AC Current Clamp	54mm ø	600V CATIII		
SM UB 1000A-1V	0.5A ~ 1000A(0.5%>10A)	15Hz ∼ 15kHz	0.5%	0.5A to 1000A AC Current Clamp	54mm ø	600V CATIII		
P32 UE 1000A-1V	5A ~ 1000A	40Hz ∼ 5kHz	1%	5 A to 1000A AC Current Clamp	83mm ø (125mm×47mm or 100m m×58mm)	600V CATIII		
P32 UE 3000A-1V	5A ~ 3000A	40Hz ∼ 5kHz	1%	5 A to 3000A AC Current Clamp	83mm ø	600V CATIII		









Current Clamp M3-UB 50A-1V

Current Clamp S-UE 200A-1V

Current Clamp SM-UB 1000A-1V

Current Clamp P32-UE 1000A-1V

Probe / Current Clamp (Hall effect): AC + DC								
Model number	Measuring range	Frequency range	Accuracy	Details	Clamp diameter	Category		
SC 2C 100A-1V	$1A \sim 100A$	DC ∼ 5kHz	2%	1A to 100A AC+DC Current Clamp	50mm ø	600V CATIII		
SC 3C 1000A-1V	$1A \sim 1000A$	DC~2kHz	1%	1A to 1000A AC+DC Current Clamp	59mm ø	600V CATIII		
P20 3C 2000A-2V	40A ~ 1000/2000A	DC ~ 2kHz	1%	40A to 2000A AC+DC Current Clamp	83mm ø	600V CATIII		
P40 3C 4000A-2V	40A ~ 2000/4000A	DC ~ 2kHz	1.5%	40A to 4000A AC+DC Current Clamp	83mm ø	600V CATIII		
P50 3C 5000A-2V	50A ~ 2000/5000A	DC ~ 2kHz	1.5%	50A to 5000A AC+DC Current Clamp	83mm ø	600V CATIII		









Current Clamp SC 2C 100A-1V

Current Clamp SC 3C 1000A-1V

Current Clamp P20 3C 2000A-2V

Current Clamp P50 3C 5000A-2V

Rogowski Current Transducers: AC							
Model number	Measuring range	Frequency range	Accuracy	Details	Coil/Through Hole Circumference	Category	
WR5000 Rogowski	1A ~ 5000A	1Hz ∼ 1MHz	0.05%	1A to 5000A AC Rogowski Coil	600mm	600V CATIII	
WR10000 Rogowski	1A ~ 10000A	1Hz ∼ 1MHz	0.05%	1A to 5000A AC Rogowski Coil	600mm	600V CATIII	



WR5000 Rogowski Coil

Zero Flux Current Transducer: AC+DC						
Model number	Measuring range	Frequency range	Accuracy	Details	Coil/Through Hole Circumference	Category
LEM IT 60-S	0A ~ 60A DC (42Arms)	DC ~ 800kHz	0.01%	60A Zero Flux Transducer	26mm	600V CATIII
LEM IT 200-S	0A ~ 200A DC (141Arms)	DC ~ 500kHz	0.01%	200A Zero Flux Transducer	26mm	600V CATIII
LEM IT 400-S	0A ~ 400A DC (282Arms)	DC ∼ 500kHz	0.01%	200A Zero Flux Transducer	26mm	600V CATIII
LEM IT 700-S	0A ~ 700A DC (495Arms)	DC ~ 100kHz	0.01%	700A Zero Flux Transducer	30mm	600V CATIII
LEM IT 1000-S	0A ~ 1000A DC (707Arms)	DC ∼ 500kHz	0.01%	1000A Zero Flux Transducer	30mm	600V CATIII
LF 510-S	0A ~ 800A DC (500Arms)	DC ~ 200kHz	0.6%	500Arms Zero Flux Transducer	30.2mm	600V CATIII
LF 1010-S	0A ~ 1500A DC (1kArms)	DC ~ 200kHz	0.4%	1kArms Zero Flux Transducer	38.5mm	600V CATIII
LEM-4	LEM-4 PPA to Transducer 4 Channel Interface Box + PSU's					



LEM IT700-S

PPA3500 SERIES MODELS

Phases	Model	Specification
1 Ph	PPA3510-LC	
2 Ph	PPA3520-LC	DC,
3 Ph	PPA3530-LC	10mHz ∼ 1MHz
4 Ph	PPA3540-LC	30mApk ∼ 300Apk
5 Ph	PPA3550-LC	(20Arms)
6 Ph	PPA3560-LC	

Phases	Model	Specification
1 Ph	PPA3510	
2 Ph	PPA3520	DC,
3 Ph	PPA3530	10mHz ∼ 1MHz
4 Ph	PPA3540	100mApk ~ 300Apk
5 Ph	PPA3550	(30Arms)
6 Ph	PPA3560	

PPA3500 SERIES UPGRADE PATH

Model	Details		
3500-CH+LC	PPA3500 Additional Input Channel (Voltage and Current) 20A		
3500-CH+	PPA3500 Additional Input Channel (Voltage and Current) 30A		

PRODUCT COMPARISON						
	PPA500	PPA1500	PPA3500	PPA4500	PPA5500	
Basic Accuracy				222	1111	
V, A rdg error	0.05%	0.05%	0.04%	0.03%	0.01%	
Power rdg error	0.10%	0.10%	0.06%	0.04%	0.02%	
Phase Options						
Internal	1~3	1~3	1~6	1~3	1~3	
Master/Slave operation	_	_	_	4~6	4 ~ 6	
Bandwidth						
20 & 30A Shunt	DC ~ 500kHz	DC ∼ 1MHz	DC ~ 1MHz	_	-	
10 & 30A Shunt	_	_	-	DC ∼ 2MHz	DC ∼ 2MHz	
50A Shunt	_	_	-	DC ∼ 1MHz	DC ∼ 1MHz	
Voltage Input						
Max input voltage	2500Vpk (1kVrms)	2500Vpk (1kVrms)	2500Vpk (1kVrms)	3000Vpk (1kVrms)	3000Vpk (1kVrms)	
No. of ranges	8	8	10	8	9	
Direct Current Input						
10Arms model	_	_	_	0	0	
20Arms model	0	0	O	_	1	
30Arms model	0	0	0	0	0	
50Arms model	_	_	_	0	0	
No. of ranges	8	8	10	8	9	
Features						
Scope and Graph Modes	_	0	0	0	0	
USB Memory port	0	0	0	0	0	
LAN Port	0	0	0	0	0	
GPIB Port	0	0	0	0	0	
RS232 Port	0	0	0	0	0	
Real time clock	0	0	0	0	0	
19in Rack mount option	0	0	<u> </u>	0	0	
Torque and Speed	_	_	0	0	0	
IEC61000 Mode	_	_	_	_	0	
PWM Motor Drive Mode	_	Limited Functionality	0	0	0	
Oscilloscope	_	0	0	0	0	
Transformer Mode	_	_	0	0	0	
PWM Filter Options	_	2	7	7	7	
Speed/Harmonics/Sec	300/sec	300/sec	300/sec	600/sec	1800/sec	
Internal Datalogging	4 Parameters	4 Parameters	32 Parameters	16 Parameters	16 Parameters	
Datalog Records	16000	16000	5M	5M	10M	
ABD0100.1.8 Mode	-	_	-	-	0	
Internal Memory	192kB	192kB	500MB	500MB	1GB	
Harmonics	50	50	100	100	417	
Minimum Window Size	10ms	5ms	5ms	2ms	2ms	
Dimensions - Excl. Feet H x W x D (mm)	92 x 215 x 312	92 x 215 x 312	92 x 404 x 346	130 x 400 x 315	130 x 400 x 315	
Weight	3.3 - 4kg	3.3 - 4kg	5 - 8.8kg	5.4 - 6kg	5.4 - 6kg	


- Not Applicable

Option

Standard

All specifications at 23° C ± 5° C. These specifications are quoted in good faith but Newtons4th Ltd reserves the right to amend any specification at any time without notice

The N4L product range also includes Frequency Response and Impedance Analyzers, Selective Level Meters and Laboratory Power





PSM17xx $10\mu Hz\sim 35MHz$

Applications

Newtons4th Ltd N4L

• Power supply phase margin and gain margin (FRA)

- Inductance, Capacitance and Resistance (LCR)
- Analysis of mechanical vibration (HARM)
- Phase Angle Voltmeter (PAV)

Contact your local N4L Distributor for further details

Newtons4th

Newtons4th Ltd (abbreviated to N4L) was established in 1997 to design, manufacture and support innovative electronic equipment to a world-wide market, specialising in sophisticated test equipment particularly related to phase measurement. The company was founded on the principle of using the latest technology and sophisticated analysis techniques in order to provide our customers with accurate, easy to use instruments at a lower price than has been traditionally associated with these types of measurements. Flexibility in our products and an attitude to providing the solutions that our customers really want has allowed us to develop many innovative functions in our ever increasing product range.





Newtons4th Ltd are ISO9001 registered, the internationally recognised standard for the quality management of businesses

THE QUEEN'S AWARDS FOR ENTERPRISE: INNOVATION

In recognition of the technical innovation and commercial success of the PPA series, N4L received the "Innovation 2010" Queen's award for enterprise

Distributed by:

Newtons4th Ltd 1 Bede Island Road Leicester LE2 7EA UK

Phone: +44 (0)116 230 1066 +44 (0)116 230 1061 Fax: Email: sales@newtons4th.com Web: www.newtons4th.com

copyright © 2010-2015 Newtons4th Document ref: 527-001/1